

Radiopacity of bulk fill flowable resin composite materials

T Yildirim, MK Ayar¹, MS Akdag, C Yesilyurt

Department of Restorative Dentistry, Faculty of Dentistry, Karadeniz Technical University, Trabzon, ¹Department of Restorative Dentistry, Faculty of Dentistry, Biruni University, Istanbul, Turkey

Abstract

Objectives: The purpose of this study was to evaluate the radiopacity of currently marketed bulk fill flowable dental composite materials (Beautiful Bulk Flowable, SDR Flow, Filtek Bulk Fill Flow, and x-tra Base Bulk Fill).

Materials and Methods: Six specimens of each material with a thickness of 1 mm were prepared, and digital radiographs were taken, using a CCD sensor along with an aluminum stepwedge and 1 mm-thick tooth slice. The mean gray level of each aluminum stepwedge and selected materials was measured, using the equal-density area tool of Kodak Dental Imaging software. The equivalent thickness of aluminum for each material was then calculated by using the stepwedge values in the CurveExpert version 1.4 program.

Results: The radiopacity of bulk fill flowable composites sorted in descending order as follows: Beautiful Bulk Flowable (2.96 mm Al) = x-tra base bulk fill (2.92 mm Al) = SureFil SDR Flow (2.89 mm Al) > Filtek Bulk Fill Flow (2.51 mm Al) ($P < 0.05$).

Conclusions: As all materials had a radiopacity greater than dentin and enamel; their adequate radiopacity will help the clinicians during radiographic examination of restorations.

Clinical Significance: Bulk fill composite materials have greater radiopacity, enabling clinicians to distinguish the bulk fill composites from dentin and enamel.

Key words: Bulk-fill flowable, composite, radiopacity

Date of Acceptance: 23-Aug-2015

Introduction

Resin composite materials have been improved significantly since they were first introduced more than a half century ago,^[1] and current resin composite materials exhibit clinical success comparable to or higher than that of dental amalgam.^[2,3] These materials are widely used in dentistry for their aesthetic and mechanical properties,

which closely resemble those of natural teeth, and for their excellent adhesion to dental hard tissues.^[4] However, the major disadvantage of current resin composite restoratives is the incremental placement technique required to reduce polymerization stress and to ensure complete depth of cure on light irradiation.^[5]

Flowable resin restoratives can be used to address some of the challenges created for dentists by placement of higher viscosity universal or posterior composites. Flowable composites have the good wetting capacity and greater ease of insertion, which helps adaptation to cavity walls

Address for correspondence:

Dr. T Yildirim,
Department of Restorative Dentistry, Faculty of Dentistry,
Karadeniz Technical University, Trabzon, Turkey.
E-mail: drtahsiny@outlook.com

Access this article online

Quick Response Code:



Website: www.njcponline.com

DOI: 10.4103/1119-3077.178919

PMID: *****

This is an open access article distributed under the terms of the Creative Commons Attribution-NonCommercial-ShareAlike 3.0 License, which allows others to remix, tweak, and build upon the work non-commercially, as long as the author is credited and the new creations are licensed under the identical terms.

For reprints contact: reprints@medknow.com

How to cite this article: Yildirim T, Ayar MK, Akdag MS, Yesilyurt C. Radiopacity of bulk fill flowable resin composite materials. Niger J Clin Pract 0;0:0.

when they are used as liners.^[6,7] However, the first flowable composites were not a suitable choice for composite restoration because of their poorer mechanical properties and high volumetric shrinkage, due mainly to the lower filler content.^[6,8]

To simplify the placing procedure for composite materials, one of the latest trends in dental materials research is the development of flowable composite materials that can be placed in bulk up to a thickness of 4 mm. Recently, several posterior bulk fill flowable composite materials with the more favorable mechanical properties than those of conventional flowable composites were introduced by a number of manufacturers. Although it was reported that bulk fill flowable composites had mechanical properties similar to those of conventional composites,^[9] previous studies reported that when bulk fill flowable resin composite restoratives were placed in a single 4 mm increment, marginal adaption,^[10] and bond strength^[11] to dentin were uninfluenced by bulk placement.

Radiopacity is one of the essential properties of all restorative materials. According to the International Standards Organization for Standardization (ISO 4049), the radiopacity of such materials should be equal to or greater than the same thickness of aluminum and should not be <0.5 mm of any value claimed by the manufacturer.^[12] Radiopacity must differ sufficiently from tooth tissue to be capable of being distinguished, and the restorative material must also be radiopaque enough to be distinguished from a void.^[13] Adequate radiopacity of the material allows the clinician to differentiate secondary caries formation from restoration and surrounding tooth structure, to evaluate and detect voids, overhangs and open margins, and to locate dental pulp on radiographs.^[14] In addition, studies conclude that, for optimum contrast, a restorative material with a radiopacity slightly greater than or equal to that of enamel is ideal for the detection of secondary caries in radiographs.^[15,16]

Although a number of studies have been conducted on the radiopacity of composite materials, at the time of this study, there was no report in the literature on the radiopacity of bulk flow composite restoratives, and dentists must, therefore, rely on manufacturers' data. As it has been shown, these data were not always reliable,^[17] the aim of the present study was to evaluate the radiopacity of bulk fill flowable composite materials by using a digital radiography system.

Materials and Methods

Specimen preparation

The materials evaluated in the present study were comparatively new, commercially available bulk fill flowable dental composite materials. The materials used are shown in Table 1. Four holes, 1 mm in depth, and 5 mm in width

were prepared on the plastic plates, 1 mm in thickness by using a puncher. After filling the holes on the plate with a material, a glass slide was used to cover the surface of each material to flatten the surface and to force out any excess material. Specimens were polymerized by use of an LED curing device (Elipar Freelight 2: 3M ESPE, St. Paul, USA) with a power of 1000 mW/cm² for 10 s. By this way, six composite discs, 1 mm in depth, and 5 mm in width were prepared for each group. Specimens with macroscopic defects (i.e., voids, cracks) were excluded from the study, and new specimens were prepared as previously described.

The thickness of each specimen was measured using a digital caliper (Mitutoyo, Tokyo, Japan) to obtain 1 mm thickness, and 600- and 1.000-grit silicon carbide papers were also used for this purpose. All bulk fill specimens were stored dry and in darkness at room temperature for 24 h prior to the performance of radiopacity measurement.

Noncarious human third molars were used for the enamel/dentin specimens. A specimen, 1 mm in thickness of was prepared by longitudinal sectioning of a third molar, using a slow-speed diamond saw (Micracut 151, Metkon, Bursa, Turkey) with a constant speed of 250–300 rpm.

Radiopacity evaluation

Digital radiographic images of the specimens were acquired by use of a Kodak digital sensor (Eastman Kodak Co., Rochester, NY) together with an aluminum stepwedge with variable thickness (from 1 to 14 mm, in 1 mm increments) and tooth slice. A Kodak 5100 intraoral X-ray unit was used, operating at 60 kV, 7 mA, and 0.20 s. The object-to-focus distance was 30 cm. Standardization of the focus-to-film distance (30 cm) and the 90° angle positions of both the digital RVG sensor and head of the X-ray machine were performed similar to Carvalho-Junior's contrivance [Figure 1].^[18]

The mean gray value of each aluminum stepwedge and selected materials was measured by outlining a region of interest, using the equal-density area tool of Kodak's Dental Imaging software version 6.12.32.0 (Eastman Kodak Co., Rochester, NY) [Figure 2]; regions were selected by avoiding areas containing air bubbles inside the material. This procedure was repeated 5 times for each specimen and aluminum stepwedge, and the average was calculated. The mean gray value of the material was then converted to millimeters of aluminum equivalent, using the CurveExpert version 1.4 program (Hyams D.G., Starkville, MS, USA). The measurement was undertaken by one operator, and the operator was blinded to the identity of the materials.

Statistical analysis

The distribution of radiopacity data were primarily analyzed for normal distribution using the Kolmogorov–Smirnov test and for equal variance using the Levene test. Although radiopacity

data were normally distributed, group variances were not equal, and nonparametric tests (Kruskal–Wallis test and Mann–Whitney U-test) were used to compare mean radiopacity across different groups. The statistical analyses were performed using SPSS version 18 software (SPSS Inc., Chicago, IL, USA). The level of significance was set at $P = 0.05$.

Results

Table 2 and Figure 3 show the mean radiopacity values of the evaluated materials, which were as follows: Beautiful Bulk Flowable (2.96 ± 0.1 mm Al) = x-tra base bulk fill (2.92 ± 0.1 mm Al) = SureFil SDR Flow (2.89 ± 0.1 mm Al) > Filtek Bulk Fill Flow (2.51 ± 0.2 mm Al). All bulk fill flowable composites had significantly greater radiopacity values than the dentine and enamel ($P < 0.05$). There were no significant differences among radiopacity values of SureFil SDR Flow, Beautiful Bulk Flowable, and x-tra base bulk fill, but the radiopacity of these materials was significantly higher than that of Filtek Bulk Fill Flow ($P < 0.05$) [Figure 3].

Table 1: Materials use in the present study

Materials	Filler% (wt/vol)	Composition
SureFil SDR Flow (Dentsply, Konstanz, Germany) Lot: 110291	64/44	Filler: Ba-Al-F-B-Si glass and St-Al-F-Si glass as fillers Resin matrix: Modified UDMA, TEGDMA, EBPDMA
Beautiful Bulk Flowable (Shofu, Kyoto, Japan) Lot: 071402	73/60	Filler: F-Al-Si glass Resin matrix: Bis-GMA, Bis-MPEPP, TMGDMA
Filtek Bulk Fill Flow (3M ESPE, Seefeld, Germany) Lot: N657914	64.5/42.5	Filler: Zirconia/silica, ytterbium Trifluoride Resin matrix: Bis-GMA, UDMA, Bis-EMA, Procrlyat resins
X-tra Base Bulk Fill (Voco, Cuxhaven, Germany) Lot: 1445154	75/61	Filler: NA Resin matrix: Bis-GMA, UDMA

NA=Not available, Bis-EMA=Bisphenol-A polyethylene glycol diether dimethacrylate, Bis-GMA=Bisphenol-A diglycidyl ether dimethacrylate, Bis-MPEPP=Bisphenol-A-Polyethoxy-Dimethacrylat, EBPDMA=Ethoxylated Bisphenol-A-dimethacrylate, TEGDMA=Triethylene glycol dimethacrylate, UDMA=Urethane dimethacrylate, TMGDMA=Tetramethylene glycol dimethacrylates

Table 2: Radiopacity of bulk-fill flowable composite materials

Material	Mean (SD) (mm eq AL)	Subset ^a	Radiopacity declared by the manufacturer
Beautiful bulk flowable	2.96 ± 0.1	a	2.5 mm Al
X-tra base bulk fill	2.92 ± 0.1	a	3.5 mm Al
SureFil SDR flow	2.89 ± 0.1	a	2.2 mm Al
Filtek bulk fill flow	2.51 ± 0.2	b	2.4 mm Al
Dentin	1.09 ± 0.0	c	
Enamel	1.84 ± 0.0	d	

^aSubsets demonstrating similar means ($P < 0.05$)

Discussion

Restorative materials should ideally be radiopaque to enable visualization and assessment by radiograph, and all newly developed materials should, therefore, be investigated in this respect.^[19] Bulk fill flowable resin composite restoratives

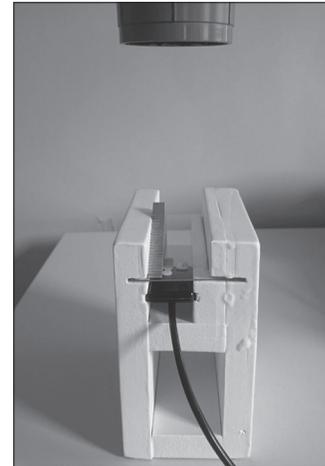


Figure 1: Front view of experimental set-up, which keeps the head of the X-ray central beam at 30 cm and at a 90° angle to the surface of CCD sensor

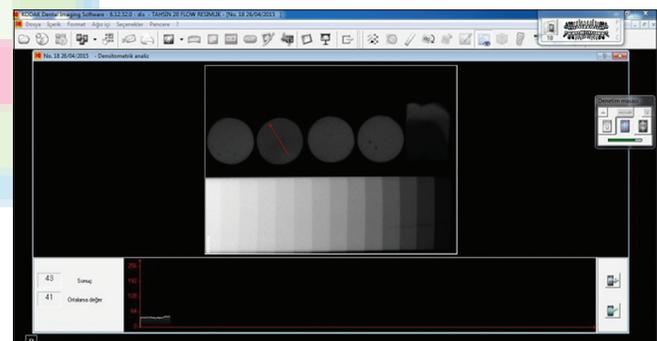


Figure 2: Screen image of computer during measurement of radiopacity of materials by Kodak Dental Imaging Software version 6.7 (Eastman Kodak Co., Rochester, NY)

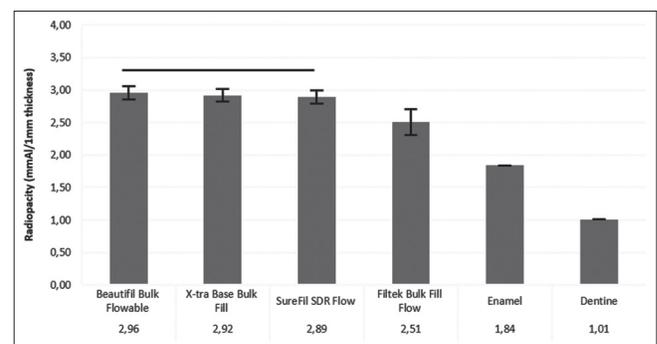


Figure 3: Mean (standard deviation) radiopacity of bulk fill flowable dental composite materials, compared to dentin and enamel. (Horizontal bars indicate that means are not significantly different from each other) ($P < 0.05$)

are relatively new to the market, but until date there are no reports in the literature about the radiopacity of these materials. For that reason, four currently available bulk fill flowable composite restoratives were evaluated in this study.

The results show that the radiopacity values of all the tested materials were greater than those of enamel and dentin, which means that none of the tested materials could be misinterpreted as dentinal caries on the radiograph. Previous studies have concluded that restorative materials with a radiopacity slightly greater than or equal to enamel is ideal for the detection of secondary caries in radiographs; these materials fulfilled this requirement and can, therefore, be used in restorative applications.^[20,21]

The reported radiopacity values of bulk fill flowable resin composite are limited in the literature, therefore, dentists have rely on only manufacturer given information. The manufacturers provided exact radiopacity values for all the tested materials were shown in Table 1. Comparing the results of this study with the radiopacity values as declared by the manufacturers, it can be seen that the value for Filtek Bulk Fill Flow accord with our results. However, there are noticeable differences between our results and the manufacturers' radiopacity values for x-tra base bulk fill (2.92/3.5 mm Al), Beautiful Bulk Flowable (2.96/2.5 mm Al, and SureFil SDR Flow (2.89/2.2 mm Al). One of the requirements of ISO 4049 is that the radiopacity of any material should not be <0.5 mm of any value claimed by the manufacturer. It follows that dentists should not rely on the radiopacity values declared by manufacturers (as also previously reported in the literature).^[17] Nevertheless, x-tra base bulk fill was found to have clinically acceptable higher radiopacities than enamel and dentin. Materials with a radiopacity close to that of dentin may present a clinical challenge for dentists during radiographic examination of restorations.

The use of 99.5% pure aluminum is currently specified when testing under the ISO Standard 4049.^[12] However, it is also advisable to use secondary standards for enamel and dentin.^[22] The dentin and enamel reference radiopacity values used in the present study were 1.09 ± 0.0 and 1.84 ± 0.0 mm Al, respectively. The values of enamel and dentin are in agreement with previous studies, where dentin radiopacity was close to 1 mm Al and enamel radiopacity was close to 2.0 mm Al.^[23-25]

In the present study, a digital radiographic system was used as it reduces the operator's (and patient's) exposure to radiation, eliminates the need for film development chemicals, offers higher resolution and greater dynamic range than X-ray film, and facilitates

image analysis. Most importantly, the digital system ensures consistent radiograph development,^[13,26] traditional film development, unless performed carefully, can produce the significant variations in the final radiograph.^[26]

Conclusion

All the tested bulk fill flowable composite materials recorded greater radiopacities than enamel and dentin. It can be concluded that these composites would not hamper radiographic examination of restorations and can be used in restorative applications. However, the evidence indicates that radiopacity data provided by manufacturers cannot be relied on in every case.

Financial support and sponsorship

Nil.

Conflicts of interest

There are no conflicts of interest.

References

1. Ferracane JL. Resin composite – State of the art. *Dent Mater* 2011;27:29-38.
2. Mair LH. Ten-year clinical assessment of three posterior resin composites and two amalgams. *Quintessence Int* 1998;29:483-90.
3. Opdam NJ, Bronkhorst EM, Loomans BA, Huysmans MC. 12-year survival of composite vs. amalgam restorations. *J Dent Res* 2010;89:1063-7.
4. Touati B, Aidan N. Second generation laboratory composite resins for indirect restorations. *J Esthet Restor Dent* 1997;9:108-18.
5. Versluis A, Douglas WH, Cross M, Sakaguchi RL. Does an incremental filling technique reduce polymerization shrinkage stresses? *J Dent Res* 1996;75:871-8.
6. Bayne SC, Thompson JY, Swift EJ Jr, Stamatias PW, Wilkerson MA. A characterization of first-generation flowable composites. *J Am Dent Assoc* 1998;129:567-77.
7. Lee IB, Min SH, Kim SY, Ferracane J. Slumping tendency and rheological properties of flowable composites. *Dent Mater* 2010;26:443-8.
8. Braga RR, Hilton TJ, Ferracane JL. Contraction stress of flowable composite materials and their efficacy as stress-relieving layers. *J Am Dent Assoc* 2003;134:721-8.
9. Ilie N, Bucuta S, Draenert M. Bulk-fill resin-based composites: An *in vitro* assessment of their mechanical performance. *Oper Dent* 2013;38:618-25.
10. Roggendorf MJ, Krämer N, Appelt A, Naumann M, Frankenberger R. Marginal quality of flowable 4-mm base vs. conventionally layered resin composite. *J Dent* 2011;39:643-7.
11. Van Ende A, De Munck J, Van Landuyt KL, Poitevin A, Peumans M, Van Meerbeek B. Bulk-filling of high C-factor posterior cavities: Effect on adhesion to cavity-bottom dentin. *Dent Mater* 2013;29:269-77.
12. International Standard 4049. Dentistry-Polymer based fillings, restorative and luting materials. Geneva: International Organisation for Standardization; 2000.
13. Nomoto R, Mishima A, Kobayashi K, McCabe JF, Darvell BW, Watts DC, *et al.* Quantitative determination of radio-opacity: Equivalence of digital and film X-ray systems. *Dent Mater* 2008;24:141-7.
14. Cook WD. An investigation of the radiopacity of composite restorative materials. *Aust Dent J* 1981;26:105-12.
15. Chan DC, Titus HW, Chung KH, Dixon H, Wellinghoff ST, Rawls HR. Radiopacity of tantalum oxide nanoparticle filled resins. *Dent Mater* 1999;15:219-22.
16. Espelid I, Tveit AB, Erickson RL, Keck SC, Glasspoole EA. Radiopacity of restorations and detection of secondary caries. *Dent Mater* 1991;7:114-7.
17. Hitij T, Fidler A. Radiopacity of dental restorative materials. *Clin Oral Investig* 2013;17:1167-77.

18. Carvalho-Junior JR, Correr-Sobrinho L, Correr AB, Sinhoreti MA, Consani S, Sousa-Neto MD. Radiopacity of root filling materials using digital radiography. *Int Endod J* 2007;40:514-20.
19. Tasdemir T, Yesilyurt C, Yildirim T, Er K. Evaluation of the radiopacity of new root canal paste/sealers by digital radiography. *J Endod* 2008;34:1388-90.
20. Goshima T, Goshima Y. Radiographic detection of recurrent carious lesions associated with composite restorations. *Oral Surg Oral Med Oral Pathol* 1990;70:236-9.
21. Altintas SH, Yildirim T, Kayipmaz S, Usumez A. Evaluation of the radiopacity of luting cements by digital radiography. *J Prosthodont* 2013;22:282-6.
22. Watts DC, McCabe JF. Aluminium radiopacity standards for dentistry: an international survey. *J Dent* 1999;27:73-8.
23. Williams JA, Billington RW. The radiopacity of glass ionomer dental materials. *J Oral Rehabil* 1990;17:245-8.
24. el-Mowafy OM, Brown JW, McComb D. Radiopacity of direct ceramic inlay restoratives. *J Dent* 1991;19:366-8.
25. Dukic W, Delija B, Derossi D, Dacic I. Radiopacity of composite dental materials using a digital X-ray system. *Dent Mater J* 2012;31:47-53.
26. Camps J, Pommel L, Bukiet F. Evaluation of periapical lesion healing by correction of gray values. *J Endod* 2004;30:762-6.

